

# Measurement Report

21/04/2004

## Patient Information

Family Name.....Brown  
 First Name.....Elaine  
 Age.....8y0m  
 Height.....  
 Weight.....

ID.....123  
 Gender.....Female  
 Date of Birth.....01/04/1996  
 Referring Physician.....  
 Reporting Physician.....  
 Operator.....sunlight



## Measurement Results

Site..... DISTAL RADIUS - Ped

SOS.....3784[m/sec]  
 Speed of Sound

Z-Score.....0.1  
 Number of standard deviations from the mean of age matched population

Percentile..... 56  
 Percentile rank to which patient belongs relative to age matched peers

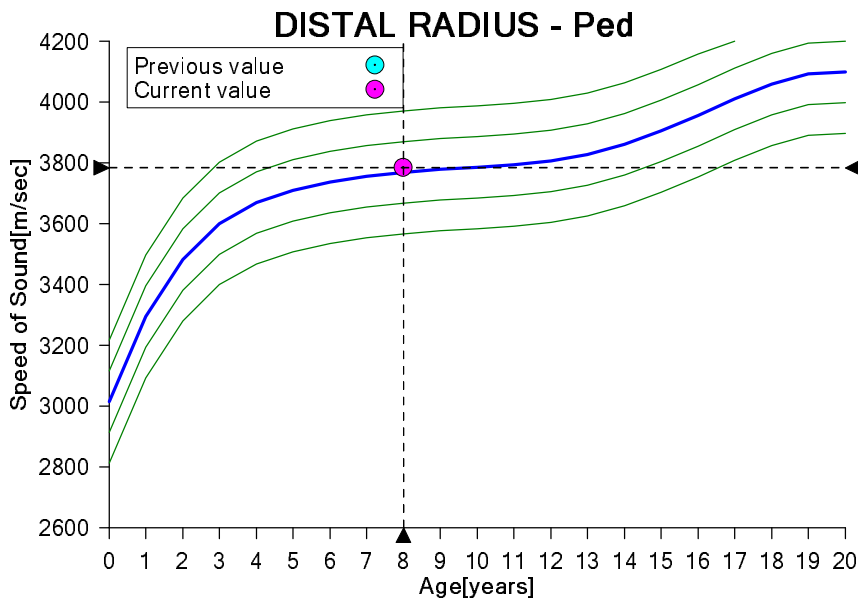

## Comments and Findings

Signature \_\_\_\_\_

## Device Details

System S/N.....22075109    Probe S/N.....CMB2058  
 S/W.....2.4.2882    Print Date.....21/04/2004  
 RDB.....Caucasian, Female

 **Sunlight Medical Ltd.**  
 Omnisense 7000P